

Fig.1

09965937.092801

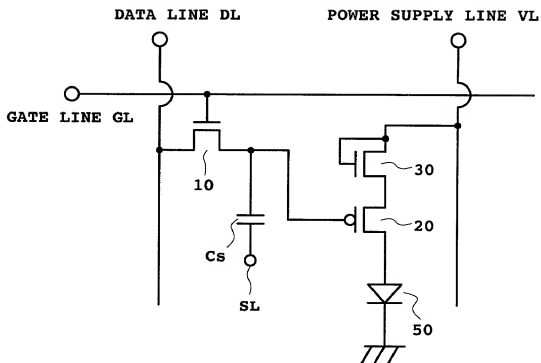


Fig.2



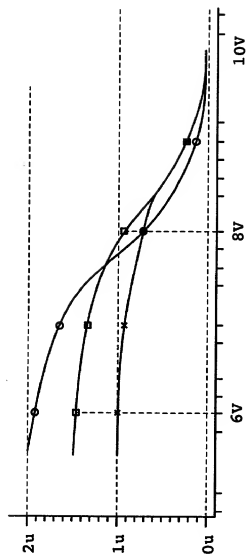


Fig. 4A

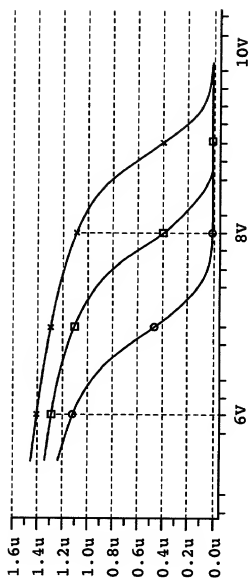


Fig. 4B


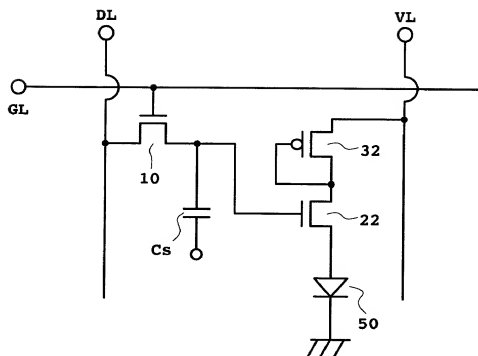


Fig.5

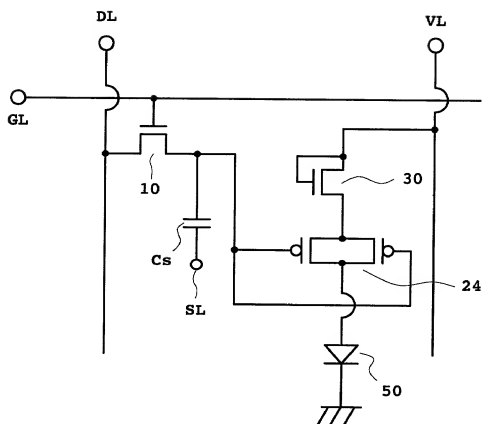

**Fig. 6**




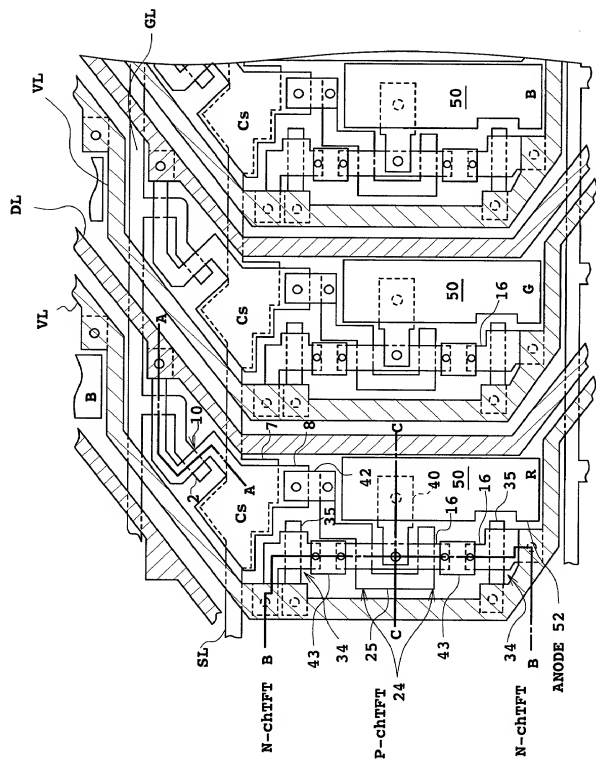


Fig. 8






↓ SCAN DIRECTION  
OF LASER ANNEAL

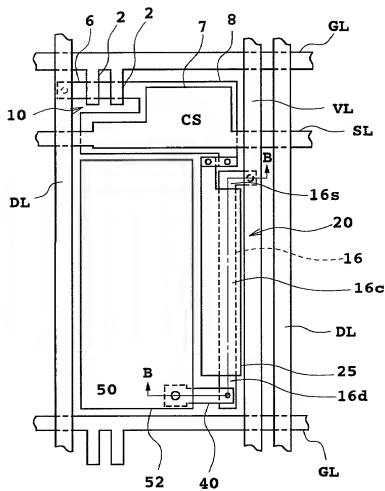

**Fig. 10A**

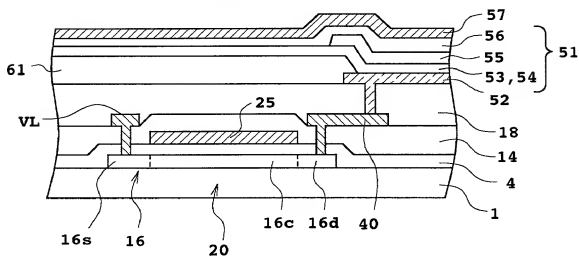

**Fig. 10B**


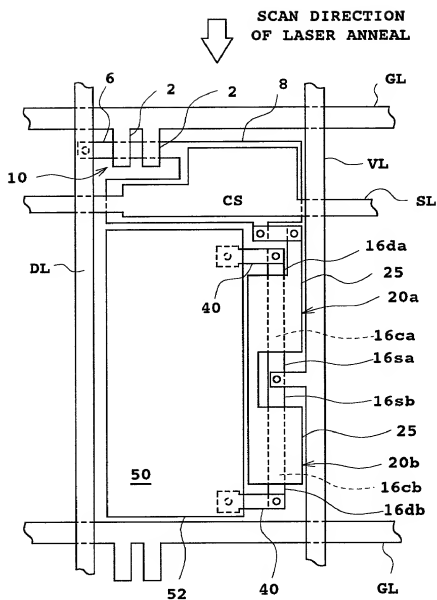



Fig.11




**Fig. 12**



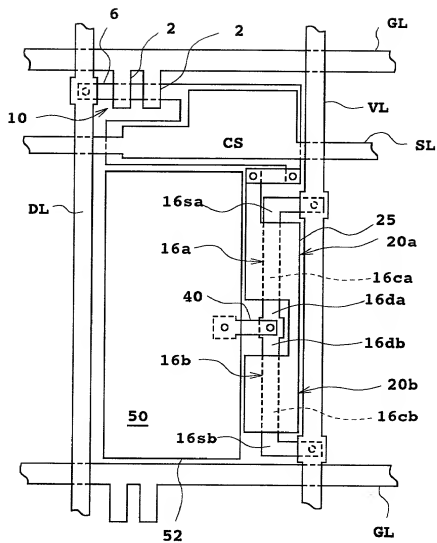

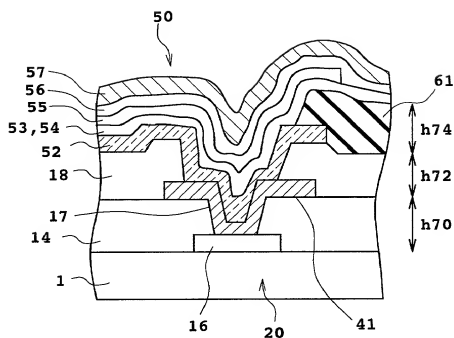

**Fig.15A**

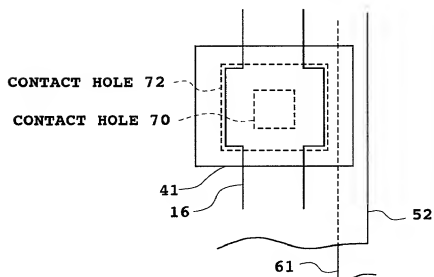

**Fig.15B**





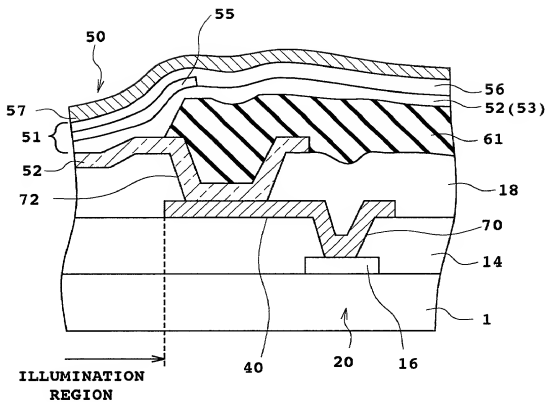


Fig. 17



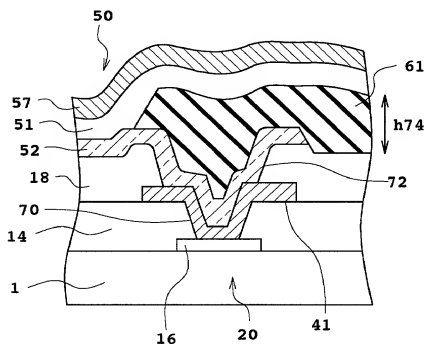


Fig. 18

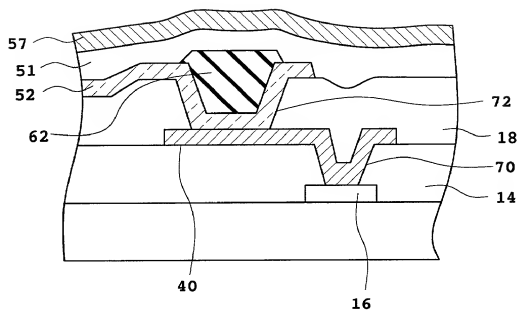

**Fig.19**

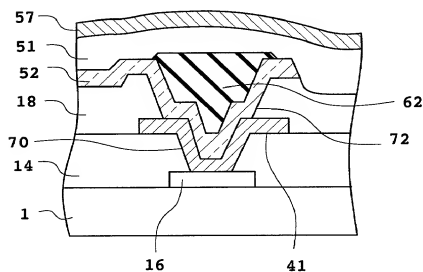

**Fig.20**